

# Vivinex™ Toric multiSert™

CLARITY & CONTROL COMBINED WITH  
OUTSTANDING ROTATIONAL STABILITY



**Vivinex™ Toric IOL** offers **clarity of vision**  
and **outstanding rotational stability**

Delivered by **multiSert™**, providing  
**unmatched control at your fingertips**

# Vivinex™ Toric

## Clarity and outstanding rotational stability


Designed for outstanding optical quality, Vivinex™ Toric multiSert™ has proven rotational stability for precise astigmatism correction and provides patients with an astigmatic cornea with clarity of vision. Product quality, dedication and attention to detail are deeply rooted in our Japanese heritage, and with 2 million lenses implanted worldwide, surgeons' trust in Vivinex™ is proven.

### Vivinex™ Toric:

- Glistening-free hydrophobic acrylic IOL material<sup>[1,2]</sup>
- Proprietary aspheric optic design for improved image quality<sup>[3]</sup>
- Active oxygen processing treatment, a smooth surface and square optic edge to reduce PCO<sup>[1,4,5,6,7,8,9,10]</sup>
- Median rotation 1.1° (range 0.0° – 5.0°)  
100% of lenses (n=103) had ≤ 5° of rotation from their initial axis at end of surgery through all follow up visits at 1 hour, 1 week, 1 month and 6 months<sup>[11]</sup>

### Textured-rough haptic surface for better grip

Vivinex™ haptics have different surface structures. They provide better grip inside the capsular bag and are designed to reduce the potential for adhesion to the optic surface.

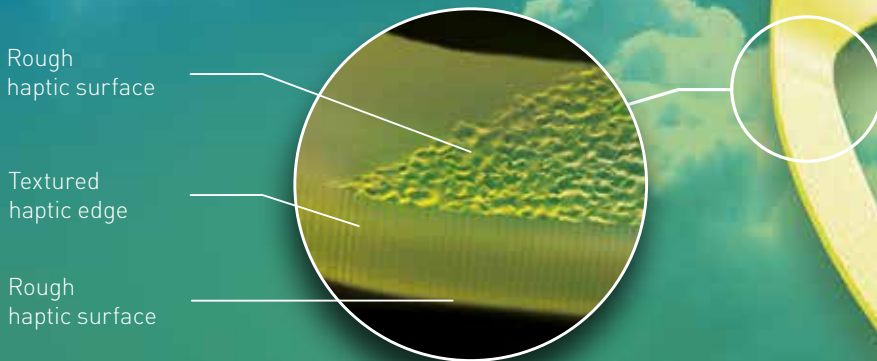


# Reliable outcomes through outstanding rotational stability<sup>[11]</sup>


Early clinical results with the Vivinex™ preloaded IOL platform at the University of Vienna confirm outstanding rotational stability. In a group of 103 eyes, no lens rotated more than 5 degrees from orientation at the end of surgery to 6 months postoperatively.

## The Vivinex™ IOL platform shows outstanding rotational stability between surgery and one week post op, without outliers, when compared to AcrySof\*, Tecnis\* and enVista\*.<sup>[11,12]</sup>

Maximum rotation values observed in the first week following surgery<sup>[11,12]</sup>

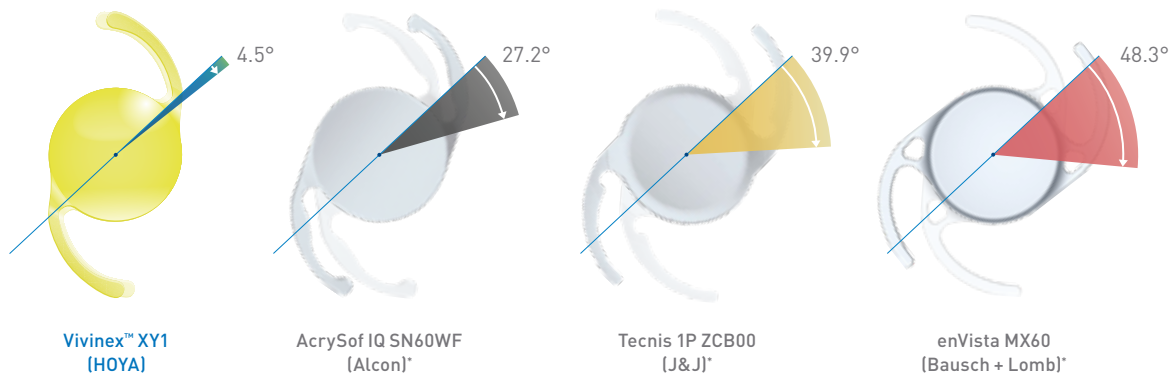

In the timeframe of up to 6 months post-op, no implanted Vivinex™ IOL rotated more than 5° from initial axis, in comparison to 4.8% of the AcrySof\* IOL, 7.5% of the Tecnis\* IOL and 13.9% of the enVista\* IOL.<sup>[11,12]</sup>

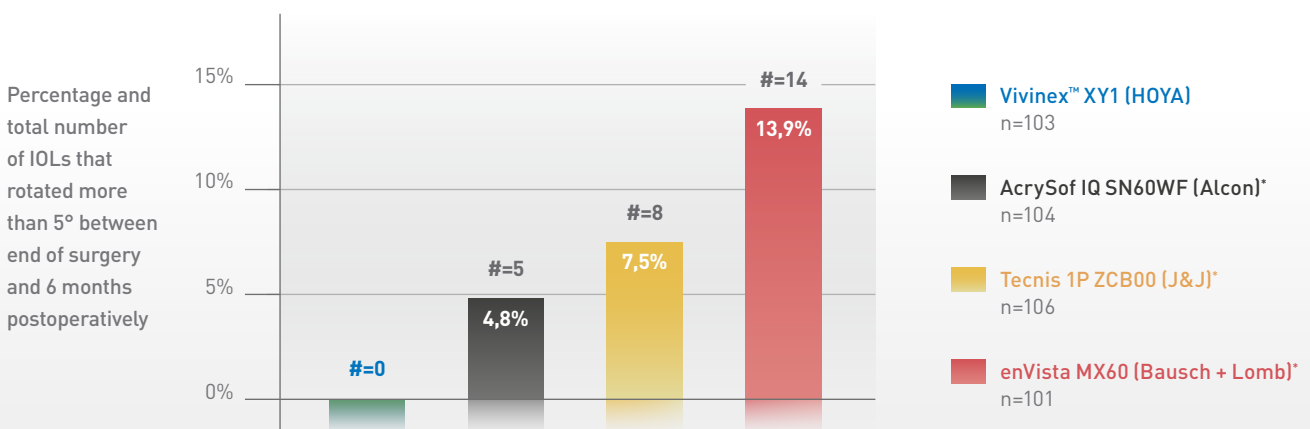


Most studies published about rotational stability of toric IOLs do not measure early rotation from the initial axis at end of surgery. The baseline for rotation measurements is often the axis of alignment at 1 day postoperative.<sup>[11,12]</sup>

## Proprietary aspheric optic design for improved image quality


In the presence of decentration Vivinex™ minimises coma when compared with other aspheric IOLs at 4.0 mm pupil diameter.<sup>[3]</sup>

Studies have shown that the mean decentration of an IOL following cataract surgery is  $0.4 \pm 0.2$  mm with a range up to 1.7 mm.<sup>[13]</sup>

### Reduced coma caused by off-axis alignment

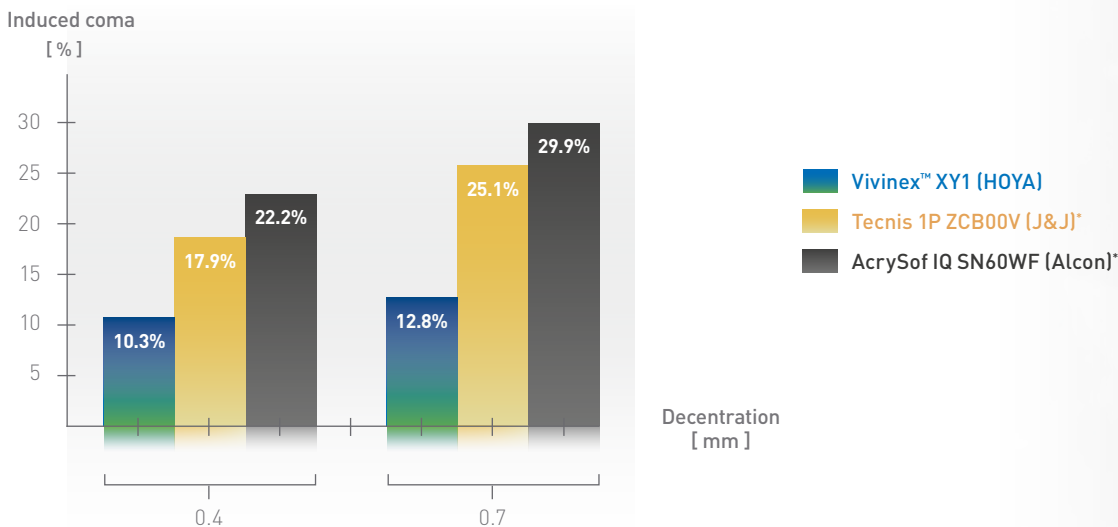

### Reduced impact on optical quality caused by off-axis alignment<sup>[3]</sup>

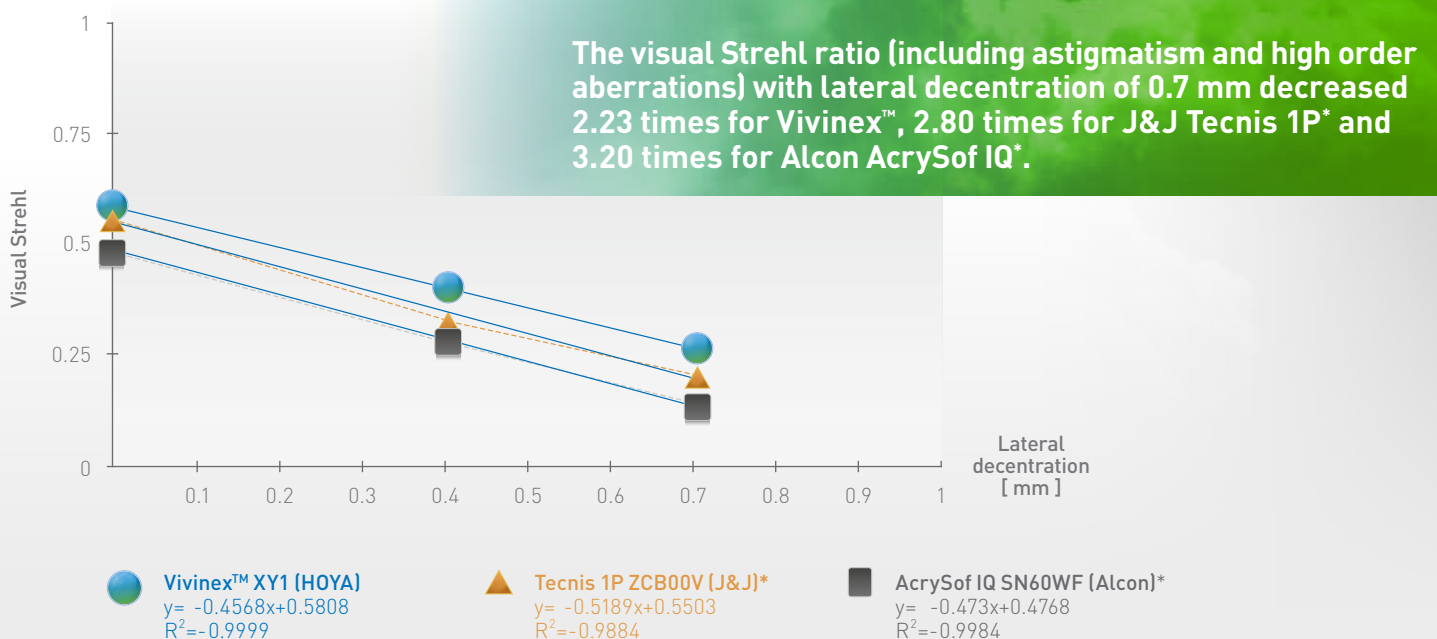

**One fits all –  
4-in-1 multiSert™ preloaded injector**



# Delivery by multiSert™, providing unmatched control at your fingertips

With multiSert™, the 4-in-1 delivery system, HOYA has developed a preloaded injector that offers the surgeon two injection options within one device. Providing single-handed push and two-handed screw injection, multiSert™ is designed to meet the surgeons' requirements and supports their personal preferences.

## Single-handed push and two-handed screw injection within one device

It's your Choice

Single-handed push injection



Two-handed screw injection



or

# Uniquely designed adjustable *insert shield* for precise injector tip insertion depth management

The innovative multiSert™ *insert shield* provides additional assurance – surgeons can modulate the insertion depth according to preference, and therefore insert the injector tip **either directly into the capsular bag or through the incision wound tunnel**: no other IOL delivery system offers this feature.



## It's your Choice

Delivery into capsular bag



or

Delivery through incision wound tunnel

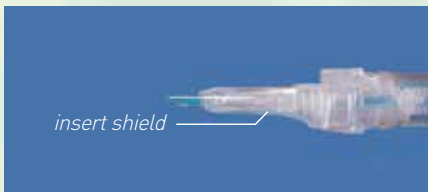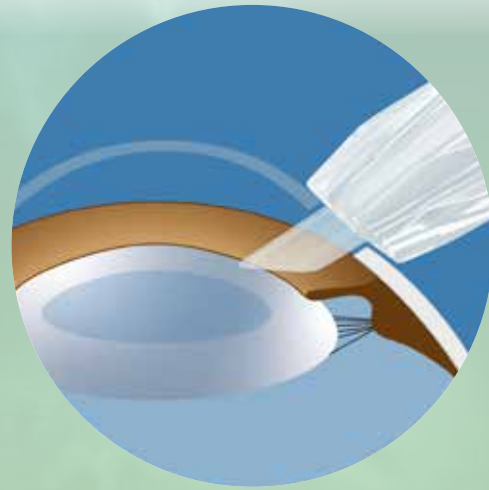


*insert shield*:  
default position




*insert shield*:  
advanced position

# multiSert™ provides outstandingly consistent and predictable IOL delivery

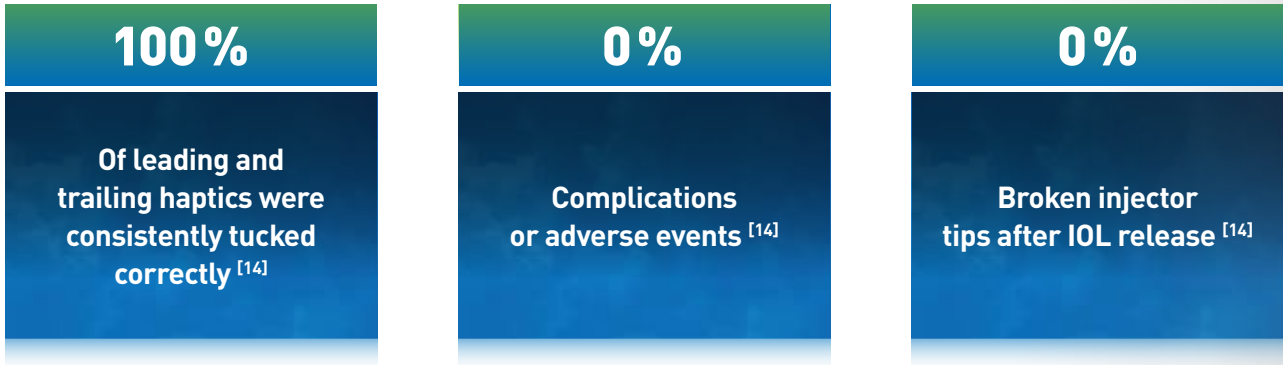

Usability and acceptability evaluation of multiSert™ was performed in the operating rooms of 14 European clinics (in Austria, France and Germany). 221 cases were completed in accordance with the instructions for use.<sup>[14]</sup>

## Ready for implantation in four easy preparation steps

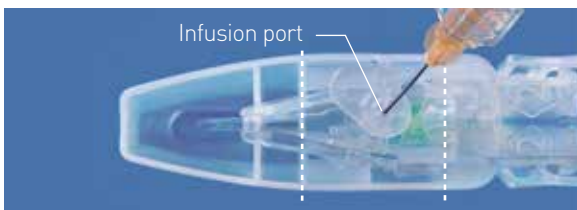


**Step 1:**  
Infuse the sodium hyaluronate OVD into the injector through the infusion port.



**Step 2:**  
Press the release tabs, lift up and remove the cover from the injector case.



**Step 3:**  
Hold injector body with thumb and slowly push the slider forward. Remove the injector from the case.

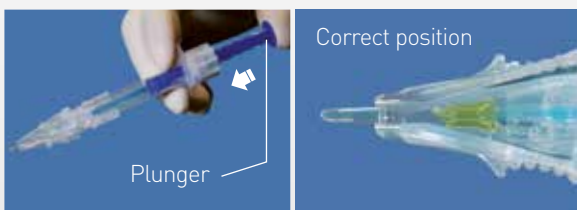

**Step 4:**  
Gently advance the plunger forward and confirm that the leading and trailing haptic are tucked correctly.

The handling shown above illustrates in summary the product application and does not replace the Instruction For Use.



# Vivinex™ Toric multiSert™

CLARITY & CONTROL COMBINED WITH  
OUTSTANDING ROTATIONAL STABILITY



## VIVINEX™ TORIC OFFERS CLARITY OF VISION AND OUTSTANDING ROTATIONAL STABILITY

- Glistening-free hydrophobic acrylic IOL material<sup>[1,2]</sup>
- Proprietary aspheric optic design for improved image quality<sup>[3]</sup>
- Active oxygen processing treatment, a smooth surface and square optic edge to reduce PCO<sup>[1,4,5,6,7,8,9,10]</sup>
- Median rotation 1.1° (range: 0.0°–5.0°)  
100% of lenses (n=103) had ≤5° of rotation from their initial axis at end of surgery through all follow up visits at 1 hour, 1 week, 1 month and 6 months<sup>[11]</sup>

## MULTISERT™ PROVIDES UNMATCHED CONTROL AT YOUR FINGERTIPS

- Single-handed push and two-handed screw injection within one device
- Uniquely designed adjustable *insert shield* for precise injector tip insertion depth management
- multiSert™ provides outstandingly consistent and predictable IOL delivery<sup>[14]</sup>

# Introducing the HOYA Toric Calculator 4



According to several studies, standard toric IOL calculations tend to result in a calculation error of astigmatic value. Most often in:<sup>[15]</sup>

- undercorrection of against-the-rule astigmatism (ATR)
- overcorrection of with-the-rule astigmatism (WTR).

The HOYA Toric Calculator (HTC) 4 can take account of posterior corneal astigmatism in the calculation by giving the option to apply the Abulafia-Koch Regression formula.


The Abulafia-Koch Regression, applied to a clinical patient cohort, has been shown to improve predictability of TIOIOL refractive outcomes.<sup>[15]</sup>

For Vivinex™ Toric IOL calculation please visit  
[\*\*www.HOYAtoric.com\*\*](http://www.HOYAtoric.com)

## The HTC 4 at a glance

- Choice of three different cylinder power options allows the doctor to select the most suitable IOL model based on residual astigmatism and axis
- Optional Abulafia-Koch Regression formula can account for the added astigmatic effect of the posterior cornea when measured by standard keratometry of the anterior corneal surface
- Option to display calculation results as plus (+) or minus (-) cylinder
- Adjustable keratometer index (default 1.3375)
- Optional axial length data entry to adjust the cylinder power of the toric IOL at the corneal plane
- Numerous different print and export options are available with customized orientation of the printed eye image

# Technical characteristics

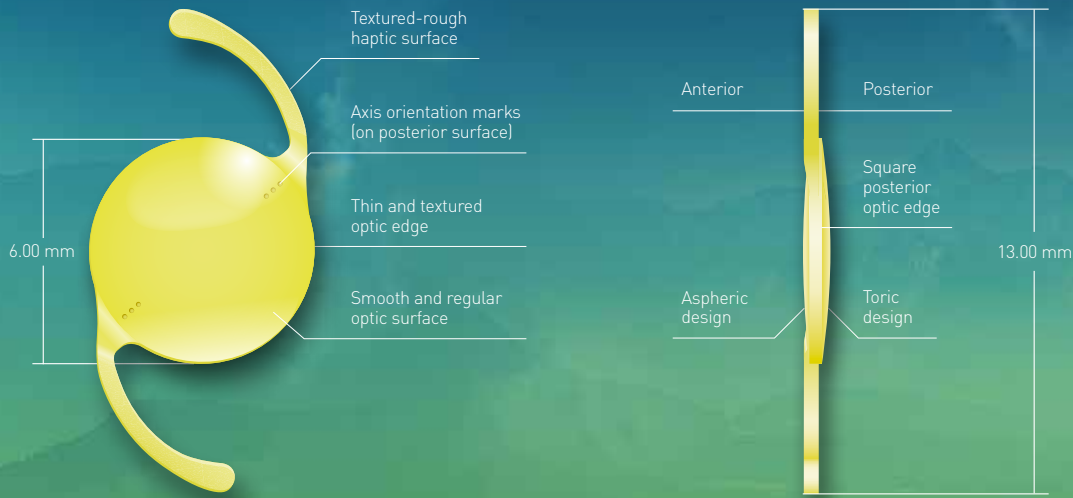

Vivinex™ Toric multiSert™	
Model name	XY1A-SP
Optic design	Biconvex with square, thin and textured optic edge Anterior: Aspheric design Posterior: Toric design
Optic & haptic materials	Hydrophobic acrylic Vivinex™ with UV- and blue light filter
Haptic design	Textured-rough haptic surface
Diameter (optic/OAL)	6.00 mm / 13.00 mm
Power	+10.00 to +30.00 D (in 0.50 D increments)
Cylinder power <sup>[16]</sup>	1.00 to 6.00 D (T2 to T9) T2 to T3 in 0.50 D increments T3 to T9 in 0.75 D increments
Nominal A-constant**	118.9
Optimized constants***	Haigis $a_0 = -0.8028$ $a_1 = 0.2133$ $a_2 = 0.2245$
	Hoffer Q     pACD = 5.697
	Holladay 1     sf = 1.934
	SRK/T     A = 119.198
Injector	multiSert™ preloaded
Front injector tip outer diameter	1.70 mm
Recommended incision size	2.20 mm

Model XY1A-SP	Cylinder power at IOL plane	Cylinder power at corneal plane <sup>[17]</sup>
T2	1.00 D	0.69 D
T3	1.50 D	1.04 D
T4	2.25 D	1.56 D
T5	3.00 D	2.08 D
T6	3.75 D	2.60 D
T7	4.50 D	3.12 D
T8	5.25 D	3.64 D
T9	6.00 D	4.17 D

\*\* The A-constant is presented as a starting point for the lens power calculation. When calculating the exact lens power, it is recommended that calculations be performed individually, based on the equipment used and operating surgeon's own experience.

\*\*\* These optimized constants for the calculation of intraocular lens power published by IOLCon on their website: <https://iolcon.org> are calculated from 1,475 clinical results for Vivinex™ Model XY1/XC1 as of September 24, 2021. These constants are based on actual surgical data and are provided by IOLCon as a starting point for individual constant optimizations. The information available on the website is based on data originating from other users and not by HOYA Surgical Optics ("HSO"). HSO therefore does not warrant the correctness, completeness and currentness of the contents on the said website.

- 1 HOYA data on file. DoF-CTM-21-002, HOYA Medical Singapore Pte. Ltd, 2021
- 2 Tandogan, T. et al. (2021): In-vitro glistening formation in six different foldable hydrophobic intraocular lenses. In BMC Ophthalmol 21, 126
- 3 Pérez-Merino, P.; Marcos, S. (2018): Effect of intraocular lens decentration on image quality tested in a custom model eye. In: Journal of cataract and refractive surgery 44 (7), p. 889–896.
- 4 Leydolt, C. et al. (2020): Posterior capsule opacification with two hydrophobic acrylic intraocular lenses: 3-year results of a randomized trial. In: American journal of ophthalmology 217 (9), p. 224–231.
- 5 Giacinto, C. et al. (2019): Surface properties of commercially available hydrophobic acrylic intraocular lenses: Comparative study. In: Journal of cataract and refractive surgery 45 (9), p. 1330–1334.
- 6 Werner, L. et al. (2019): Evaluation of clarity characteristics in a new hydrophobic acrylic IOL in comparison to commercially available IOLs. In: Journal of cataract and refractive surgery 45 (10), p. 1490–1497.
- 7 Nanavaty, M. et al. (2019): Edge profile of commercially available square-edged intraocular lenses: Part 2. In: Journal of cataract and refractive surgery 45 (6), p. 847–853.
- 8 Matsushima, H. et al. (2006): Active oxygen processing for acrylic intraocular lenses to prevent posterior capsule opacification. In: Journal of cataract and refractive surgery 32 (6), p. 1035–1040.
- 9 Farukhi, A. et al. (2015): Evaluation of uveal and capsule biocompatibility of a single-piece hydrophobic acrylic intraocular lens with ultraviolet-ozone treatment on the posterior surface. In: Journal of cataract and refractive surgery 41 (5), p. 1081–1087.
- 10 Eldred, J. et al. (2019): An In Vitro Human Lens Capsular Bag Model Adopting a Graded Culture Regime to Assess Putative Impact of IOLs on PCO Formation. In: Investigative ophthalmology & visual science 60 (1), p. 113–122.
- 11 Schartmüller, D. et al. (2019): True rotational stability of a single-piece hydrophobic intraocular lens. In: The British journal of ophthalmology 103 (2), p. 186–190.
- 12 Schartmüller, D. et al. (2020): Comparison of Long-Term Rotational Stability of Three Commonly Implanted Intraocular Lenses. In American journal of ophthalmology 220, pp. 72–81.
- 13 Harrer, A. et al. (2017): Variability in angle  $\kappa$  and its influence on higher-order aberrations in pseudophakic eyes. In: Journal of cataract and refractive surgery 43 (8), p. 1015–1019.
- 14 HOYA data on file. DoF-SERT-102-MULT-03052018, HOYA Medical Singapore Pte. Ltd, 2018
- 15 Abulafia, A. et al. (2016): New regression formula for toric intraocular lens calculations. In: Journal of cataract and refractive surgery 42 (5), p. 663–671.
- 16 At IOL plane.
- 17 Based on an average pseudophakic human eye.
- \* Third-party trademarks used herein are the property of their respective owners.

Information contained is intended for health care professionals. For a full list of indications and contra indications please refer to the Instructions For Use. Some of the products and/or specific features as well as the procedures featured in this document may not be approved in your country and thus may not be available there. Design and specifications are subject to change without prior notice as a result of ongoing technical development. Please contact our regional representative regarding individual availability in your country. HOYA, Vivinex and multiSert are trademarks of the HOYA Corporation or its affiliates.

©2021 HOYA Medical Singapore Pte. Ltd. All rights reserved.



HOYA Medical Singapore Pte. Ltd | 455A Jalan Ahmad Ibrahim | Singapore 639939



HOYA Surgical Optics GmbH | De-Saint-Exupéry-Straße 10 | 60549 Frankfurt am Main | Germany  
Hotline DE: Tel. +49 (0)800 664 2 664 | Fax +49 (0)800 774 2 774

[hoyasurgicaloptics.com](http://hoyasurgicaloptics.com)



0123 2021-09-27\_HSOE\_XY1A-SP\_BR\_EN

**HOYA**  
SURGICAL OPTICS